






Preparation

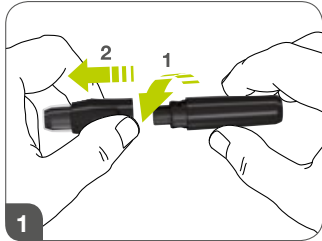


1 Twist and remove cap.

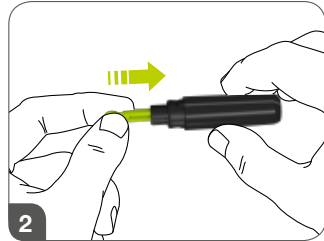


2 Insert new lancet.

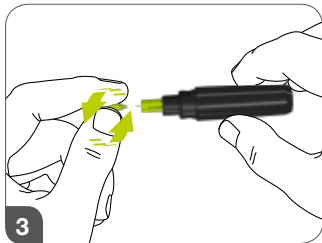


3 Twist off protective lancet cap.

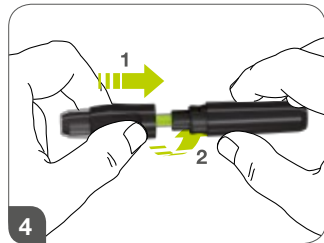

4 Replace cap and twist.

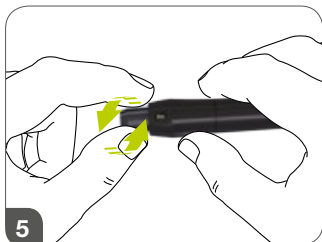

5 Set lancing depth.

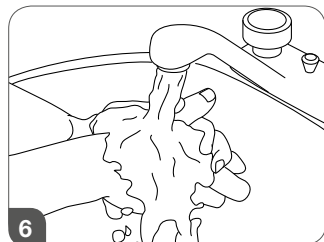


6 Wash and dry hands.




Blood sugar measurement



1 Remove test strip and re-close box.

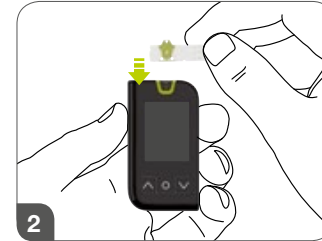


2 Insert test strip. The mylife™ Unio™ blood glucose meter starts automatically.

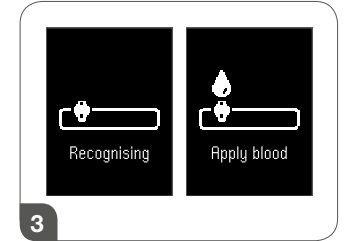


3 Wait until the symbol "Apply blood" appears.




4 Keep safety button pressed down. Then press finger onto the cap of the lancing device – Keep thumb pressed (it is not necessary to tighten).

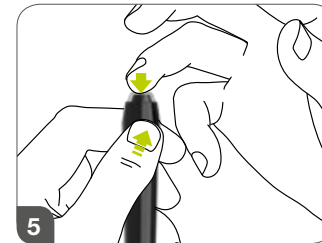

5

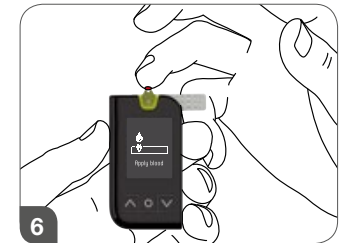

6 Apply blood.

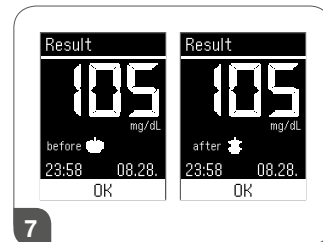

7 The reading can be directly assigned a marker (before/after meal) using the up/down buttons.



8 Hygienic removal of the test strip without blood contact.